



 **EPA USEPA Manual of  
Methods for Virology**

Chapter 14  
April 2001



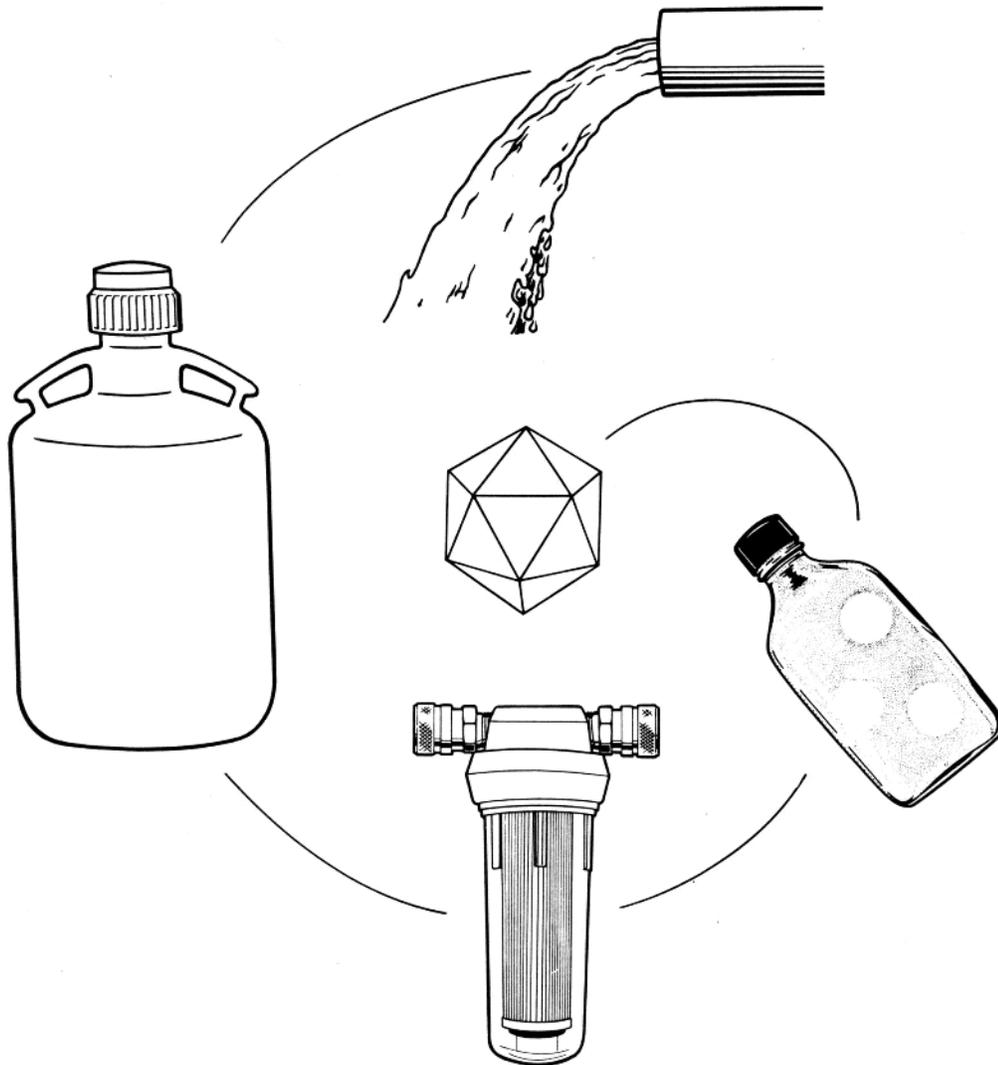

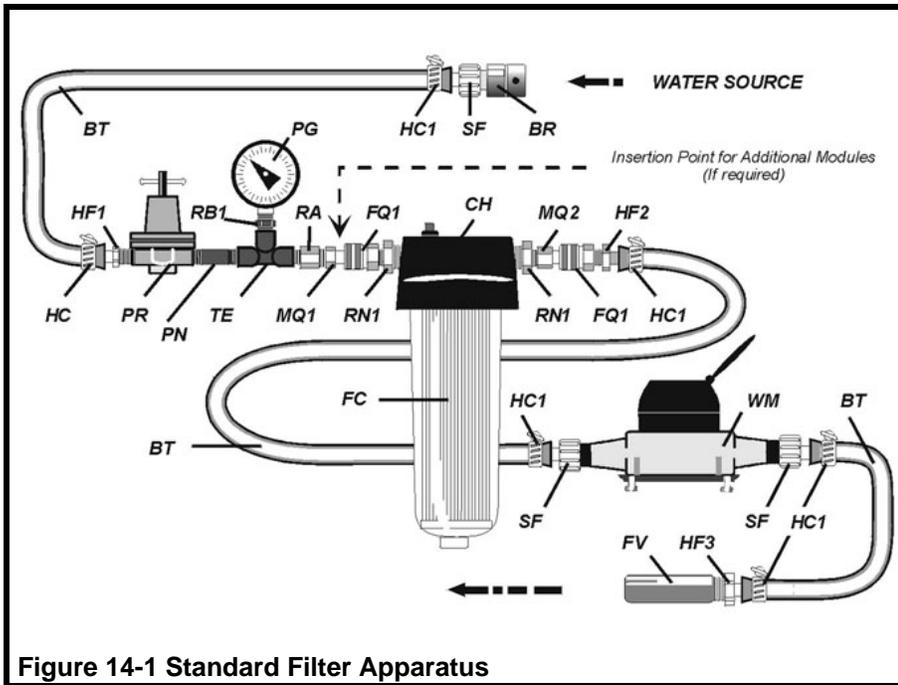

**Figure 14-1 Standard Filter Apparatus**

mer Product No. P-68004-03; place in 1/4" gauge port if using the 263A regulator).

(a.11) One RA — **Reducing Adaptor**, 1/2" female NPT × 1/2" male NPT (Cincinnati Valve and Fitting Product No. SS-8-RA-6).

(a.12) One MQ1 — **Male Quick Connect**, 1/2" male NPT (Cincinnati Valve and Fitting Product No. SS-QF8-S-8PM or Cole-Parmer Product No. P-31303-36; appropriate hose fittings and braided tubing can be substituted for quick connects).

(a.13) Two FQ1 — **Female Quick Connects**, 1/2" female NPT (Cincinnati Valve and Fitting Product No. SS-QF8-B-8PF; Cole-Parmer Product No. P-31303-01 may be used by substituting the two reducing nipples (item a.14) for two reducing bushings (3/4" male NPT × 1/2" female NPT; Cole-Parmer Product No. P-06349-35)).

(a.14) Two RN1 — **Reducing Nipples**, 3/4" male NPT × 1/2" male NPT (Cole-Parmer Product No. P-06349-87).

(a.15) One CH — **Cartridge Housing with wench** (Cuno Product No. AP11T or 44857-05).

(a.16) One FC — **Filter Cartridge**, positively charged IMDS, ZetaPor Virosorb (Cuno Product No. 45144-01-1MDS).

(a.17) One MQ2 — **Male Quick Connect**, 1/2" female NPT (Cincinnati Valve and Fitting Product No. SS-QF8-S-8PF; Cole-Parmer Product No. P-31303-36 may be used by substituting the hose fitting (item a.18) for a 1/2" female NPT × 1/2" tubing ID hose fitting (Cole-Parmer Product No. P-06464-10)).

(a.18) One HF2 — **Hose Fitting**, 1/2" male NPT × 1/2" tubing ID (United States Plastic Product No. 62142).

(a.19) One WM — **Water Meter** (Nep-tune Equipment Product No. 6" Trident 10).

*The water meter should be used in a horizontal position and protected from freezing. The order should specify that meters be rated in gallons (1 gal = 0.1337 ft<sup>3</sup> or 3.7854 L). If not specified, meters may be rated in cubic feet (1 ft<sup>3</sup> = 7.481 gal or 28.316 L).*

(a.20) One HF3 — **Hose Fitting**, nylon, 3/4" male NPT × 1/2" tubing ID (United States Plastic Product No. 61143).

(a.21) One FV — **Flow Control Valve** (Plast-O-Matic Valves Product No. FC075B-3-PVC).

(b) Apparatus assembly


*The standard filter apparatus consists of three modules: the regulator module, the cartridge housing module and the discharge module.*

*Teflon tape (Cole-Parmer Product No. P-08782-27) must be used on all threaded, non-compression fittings.*

(b.1) Regulator module — in order, as shown in **Figure 14-1**, connect the backflow regulator (BR) to a swivel female insert (SF). Clamp a piece of braided tubing (BT) onto the tubing connector of the swivel female insert using a hose clamp (HC1). Clamp the other end of the tubing to a 1/2" hose fitting (HF1). Screw the fitting into the inlet of the pressure regulator (PR). Connect the outlet of the pressure regulator to the PVC TEE (TE) via a PVC nipple (PN). Connect the pressure gauge (PG) to the top of the PVC TEE using the reducing bushing (RB1). Attach a reducing adaptor (RA) to the remaining connection on the PVC TEE. Add a male quick connect (MQ1) to the reducing adaptor.

(b.2) Cartridge housing module — Attach a female quick connect (FQ1) to a reducing nipple (RN1). Connect the reducing nipple to the inlet of the cartridge housing (CH). Attach another reducing nipple to the outlet of the housing. Attach a male quick connect (MQ2) to the reducing adaptor.

(b.3) Discharge module — attach a female quick connect (FQ1) to a hose fitting (HF2). Connect a piece of braided tubing (BT) to the hose fitting (HF2) with a hose clamp (HC1). Clamp the other end of the braided tubing to a swivel female insert (SF) with another hose clamp (HC1). Attach the swivel female insert (SF) to the inlet of the water meter (WM). Attach another swivel female insert (SF) to the outlet of the water meter (WM) and connect a piece of braided tubing (BT) with a hose clamp (HC1). Clamp the other end of

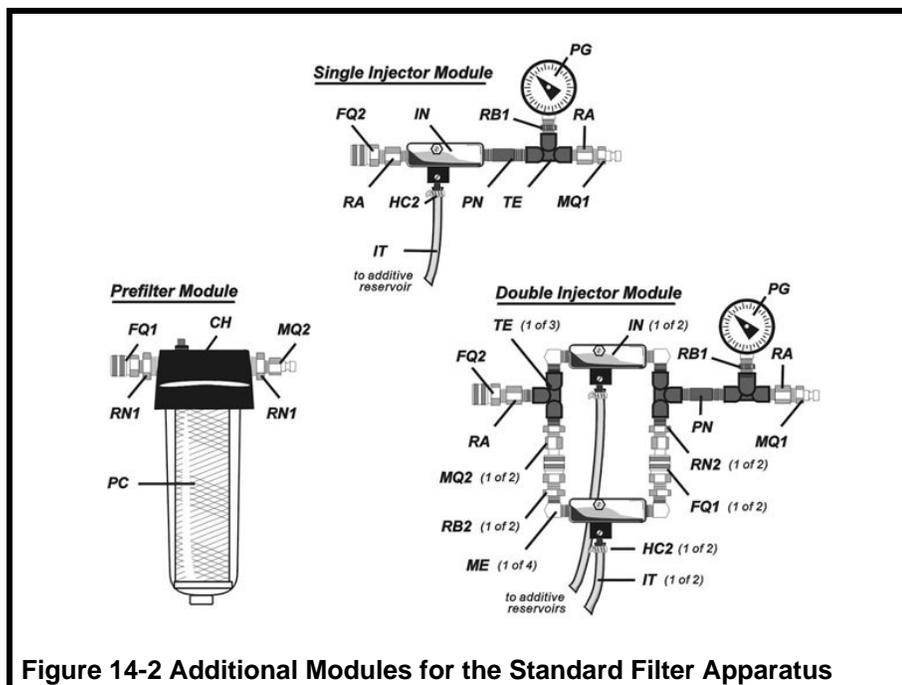

**Figure 14-2 Additional Modules for the Standard Filter Apparatus**

the tubing to a hose fitting (HF3) with another hose clamp (HC1). Screw the hose fitting (HF3) into the inlet of the flow control valve (FV). An additional hose fitting (not shown) may be added to the flow control valve for the attachment of a sufficient length of tubing to reach a drain. The discharge module does not have to be sterilized.

(b.4) Connect the cartridge housing module to the regulator module at the quick connect. The combined regulator and cartridge housing modules should be sterilized with chlorine as described in section 2.1.1a.10, 2.3.2. Presterilize a 1MDS filter cartridge (FC) as described in section 2.3.1 and place it into the cartridge housing using aseptic technique. Replace the housing head of the cartridge housing and tighten with a cartridge housing wrench. Check to ensure that the filter is adequately sealed by shaking the housing. Adequately sealed filters should not move. For convenience during shipping, the regulator and cartridge housing modules may be separated. Seal all openings into the modules with sterile aluminum foil.

### 2.1.2 Prefilter module (see **Figure 14-2**)

*Use the prefilter module for waters exceeding 75 nephelometric turbidity units (NTU) or for other conditions that prevent the minimum sampling volumes from being obtained.*

(a) Additional materials: One PC — 10  $\mu$ m Polypropylene Prefilter Cartridge (Parker Hannifin Product No. M19R10-A); in addition, a female quick connect (FQ1), two reducing nipples (RN1), a cartridge housing (CH) and a male quick connect (MQ2) as described for the standard apparatus are needed.

(b) Module assembly — in order, as shown for the prefilter module in **Figure 14-2**, attach a female quick connect (FQ1) to a reducing nipple (RN1). Connect the reducing nipple to the inlet of the cartridge housing (CH). Attach another reducing nipple to the outlet of the housing. Attach a male quick connect (MQ2) to the reducing adaptor. Sterilize the unit with chlorine as described in section 2.1.1a.10, 2.3.2 and add a presterilized polypropylene prefilter cartridge using aseptic technique.

Cover the ends with sterile aluminum foil.

### 2.1.3 Injector modules (see **Figure 14-2**)

*Use injector modules for source or finished water requiring pH reduction and for finished waters requiring dechlorination. Both single and double injector modules should be assembled so that they will be available on demand.*

(a) Materials:

(a.1) Two FQ2 — **F**emale **Q**uick **C**onnects,  $\frac{1}{2}$ " male NPT (Cincinnati Valve and Fitting Product No. SS-QF8-B-8PM).

(a.2) Four ME — **M**ale **E**lbows,  $\frac{1}{2}$ " male NPT (Cincinnati Valve and Fitting Product No. SS-6-ME).

(a.3) Two RN2 — **R**educing **N**ipples,  $\frac{1}{2}$ " male NPT  $\times$   $\frac{1}{2}$ " male NPT (Cole-Parmer Product No. P-06349-85).

(a.4) Two RB2 — **R**educing **B**ushings,  $\frac{1}{2}$ " female NPT  $\times$   $\frac{1}{2}$ " male NPT (Cole-Parmer Product No. P-06349-34).

(a.5) Three IN — **I**n-line **I**njectors (DEMA Engineering Product No. 203B  $\frac{1}{2}$ " female NPT; a metering or peristaltic pump and appropriate connectors may be substituted for an injector).

*The use of injectors significantly reduces the cost per apparatus. Injectors can be used in the absence of an electricity source, but are much more difficult to control than pumps. If pumps are selected, use a check valve (e.g., Cole-Parmer Cat. No. P-98676-00) on tubing between the pump and the main body of the module.*

(a.6) Three HC2 — **H**ose **C**lamps (Cole-Parmer Product No. P-06403-10).

(a.7) In addition to the items specified in sections 2.1.3a.1 to 2.1.3a.6, four reducing adaptors (RA), four PVC TEEs (TE), two PVC nipples (PN), two reducing bushings (RB1), two pressure

gauges (PG), two female quick connects (FQ1), two male quick connects (MQ1) and two male quick connects (MQ2) as described for the standard apparatus are needed. Two union ball joints, 1" female NPT (not shown; Cincinnati Valve and Fitting Product No. SS-6-UBJ) and two PVC nipples may be used in place of the two reducing nipples (RN2), male quick connects (MQ2), female quick connects (FQ1) and reducing bushings (RB2) used with the double injector module.

(b) Module assembly:

(b.1) Single Injector Module — assemble the parts in order as shown for the single injector module in **Figure 14-2**. Attach a female quick connect (FQ2) to a reducing adaptor (RA). Connect the adaptor to the inlet of the injector (IN). Connect the outlet of the injector to a PVC TEE (TE) via a PVC nipple (PN). Connect a pressure gauge (PG) to the top of the PVC TEE using a reducing bushing (RB1). Attach a reducing adaptor (RA) to the remaining connection on the PVC TEE. Add a male quick connect (MQ1) to the reducing adaptor.

(b.2) Double Injector Module — assemble the parts as shown for the double injector module in **Figure 14-2**. Assemble the main portion by attaching a female quick connect (FQ2) to a reducing adaptor (RA). Connect the adaptor to the top connector of a PVC TEE (TE). Add a male elbow (ME) to one of the connections on the PVC TEE. Attach a reducing nipple (RN2) to the other connection. If using a union ball joint in place of the quick connects, attach a PVC nipple (not shown) to the other connection. Add a male quick connect (MQ2) to the reducing nipple or add one portion of a union ball joint (not shown) to the PVC nipple. Connect the inlet side of an injector (IN) to the male elbow. Attach another male elbow to the outlet of the injector. Connect the male elbow to another PVC TEE. Connect a reducing nipple (RN2 or PVC nipple) to the other end of the second PVC TEE. Add a male quick

connect (MQ2) to the reducing nipple as above (or add one portion of the second union ball joint to the PVC nipple). Connect the top connector of the second PVC TEE to a third PVC TEE via a PVC nipple (PN). Connect a pressure gauge (PG) to the top of the third PVC TEE using a reducing bushing (RB1). Attach a reducing adaptor (RA) to the remaining connection on the third PVC TEE. Add a male quick connect (MQ1) to the reducing adaptor. Attach two male elbows (ME) to the inlet and outlet of a second injector (IN). Connect two reducing bushings (RB2) or, if used, the bottom portion of the two union ball joints (not shown) to the male elbows. Connect a female quick connect (FQ1) to each reducing bushing. Orient the second injector so that the direction of flow is the same as the first injector (the arrows on the injectors should both point towards the pressure gauge side of the assembly). Connect the two female quick connects to the male quick connects of the main portion to complete the assembly or, if used, connect the two portions of the union ball joints.

#### 2.1.4 Other Sampling Materials

- (a) Portable pH probe (Omega Product No. PHH-1X)
- (b) Portable temperature probe (Omega Product No. HH110).
- (c) Commercial ice packs (Cole-Parmer Product No. P-06346-76).
- (d) One liter polypropylene wide-mouth bottles (Nalgene Product No. 2104-0032).
- (e) Insulated shipping box with carrying strap (17" × 17" × 16"; Cole-Parmer Product No. P-03742-00 and P-03742-30).
- (f) Miscellaneous — aluminum foil, data card (see Appendix 2), hosecock clamp, surgical gloves, screwdriver or pliers for clamps, waterproof marker.
- (g) Chemical resistant pump capable of supplying 30 PSI at 3 gal/min and ap-

propriate connectors (for use where garden hose-type pressurized taps for the source or finished water to be monitored are unavailable and for QC samples). Follow the manufacturer's recommendations for pump priming.

## 2.2 Media and Reagents for Sampling Apparatus

**2.2.1** 0.52% chlorine (HOCl; 5250 mg/L) — add 100 mL of household bleach to 850 mL of dH<sub>2</sub>O and adjust the pH of the solution to 6-7 with 1 M HCl. Bring to 1 liter with dH<sub>2</sub>O. Store for up to two weeks at room temperature.

**2.2.2** 2% sodium thiosulfate (Na<sub>2</sub>S<sub>2</sub>O<sub>3</sub>) — dissolve 100 g of Na<sub>2</sub>S<sub>2</sub>O<sub>3</sub> in a total of 5000 mL dH<sub>2</sub>O to prepare a stock solution. Autoclave for 30 min at 121°C.

**2.2.3** Hydrochloric acid (HCl) — Prepare 0.1, 1 and 5 M solutions by mixing 50, 100 or 50 mL of concentrated HCl with 4950, 900 or 50 mL of dH<sub>2</sub>O, respectively.

*HCl solutions are self-sterilizing, therefore, prepare those solutions to be used for adjusting the pH of water samples at least 24 h before use.*

## 2.3 Sterilization of Sampling Apparatus

**2.3.1** 1MDS filter cartridges and prefilter cartridges — Presterilize 1MDS filter cartridges and prefilter cartridges by wrapping the filters in Kraft paper and autoclaving at 121°C for 30 min.

**2.3.2** Chlorine Sterilization — Sterilize pumps, sampling apparatus modules, injector tubing and plastic bags for transporting injector tubing by recirculating or immersing the items in 0.52% chlorine for 30 minutes. Drain the chlorine from the objects being sterilized. Dechlorinate by recirculating or immersing the items in a solution containing 25 mL of 2% thiosulfate per liter of sterile dH<sub>2</sub>O. Cover the apparatus module ends and the injector port(s) with sterile aluminum foil. Place the



slightly to allow it to turn freely and connect the backflow regulator to the tap. Retighten the swivel female insert. Disconnect the cartridge housing module at the quick connect (MQ1/FQ1), if connected, and cover the open end with sterile foil.

**3.1.2** Remove the foil from the ends of the discharge module and connect it to the regulator module. Place the control flow valve or tubing connected to the outlet of the flow control valve into a one liter plastic bottle. Note that the injector module, the prefilter module and the cartridge housing module must not be attached to the apparatus at this stage of the procedure!

**3.1.3** Slowly turn on the tap and adjust the pressure regulator until the pressure gauge on the regulator module reads 30 PSI (see **Figure 14-5**). If the tap is incapable of 30 PSI, adjust the regulator to achieve the maximum pressure. Pressures less than 30 PSI will result in a reduced flow rate and thus longer sampling times. Flush the apparatus assembly with at least 20 gal of the water to be sampled. While the system is being flushed, measure the pH, the temperature and the turbidity on the water collecting in and overflowing from the one liter plastic bottle. Record the values onto a sample data sheet (see Appendix 2 for an example).

*The pH meter should be calibrated before each use for the pH range of the water to be sampled.*



**Figure 14-5 Pressure Adjustment**

**3.1.4** If the sample has a pH above 8.0 or contains a disinfectant, turn off the water at the tap and disconnect the discharge module from the regulator mod-

ule. Remove the foil from the ends of a single injector module (see **Figure 14-2**) and connect the module to the male quick connect of the regulator module. Reattach the discharge module.

**3.1.5** If the sample has a pH above 8.0 and contains a disinfectant, turn off the water at the tap and disconnect the discharge module from the regulator module. Remove the foil from the ends of a double injector module (see **Figure 14-2**) and connect the module to the male quick connect of the regulator module. Reattach the discharge module.

**3.1.6** If an injector module has been added, remove the foil from the injector port(s) and attach the injector tubing to each port. Add a hosecock clamp to each injector tubing and tighten completely to prevent flow into the injector(s). Turn the fine metering adjustment screw on each injector (the smaller screw) clockwise as far as it will go to minimize the flow rate until the injectors are adjusted (note that the injectors were designed to have a minimum flow rate of 20-30 mL/min; thus completely closing the fine metering adjustment screw does not stop the flow). Place the other end of each tubing into the appropriate sterile graduated container containing 0.1 M HCl or 2% thiosulfate. Take care not to touch or contaminate the surfaces of the injector tubing that will be placed in the graduated containers. Slowly turn on the tap again and readjust the pressure regulator, if necessary.

**3.1.7** If a single injector module has been added, continue to flush the apparatus and adjust the water bypass screw on the injector (the larger adjustment screw) until the pressure gauge on the injector module is about 35% less than the pressure gauge on the regulator module (e.g., 19 PSI when the gauge on the regulator module reads 30 PSI; a minimum of a 35% pressure drop is required to achieve suction). Loosen the hosecock clamp and observe whether suction is occurring. If not, slowly increase the pressure drop until suction starts.

(a) If the pH value of the water sample is greater than 8.0, ensure that the injector or tubing is placed into a graduated container containing 0.1 M HCl. While continuing to measure the pH in the one liter plastic bottle, adjust the fine metering adjustment screw on the injector to add sufficient HCl to give a pH of 6.5 to 7.5. It may be necessary to use the hosecock clamp to reduce the flow rate to less than 20-30 mL/min or to use a more dilute or concentrated HCl solution with some water samples. When the pH stabilizes at a pH of 6.5 to 7.5, continue with step 3.1.9. Record the adjusted pH onto a sample data sheet (see Appendix 2).

(b) If the water to be sampled contains a disinfectant, ensure that the injector tubing is placed into a graduated container containing 2% thiosulfate. Adjust the fine metering adjustment screw on the injector to add thiosulfate at a rate of 10 mL/gal (2.6 mL/L or 30 mL/min at a flow rate of 3 gal/min; note that at this rate, approximately 3-4 L of thiosulfate solution will be required per sample). When the proper rate is achieved, record the presence of the disinfectant and the addition of thiosulfate on a sample data sheet (see Appendix 2) and continue with step 3.1.9.

**3.1.8** If a double injector module is being used (see **Figure 14-6**), continue to flush the apparatus and turn the water bypass screws on each injector clockwise as far as possible. Then turn the water bypass screws on each regulator one half turn counter clockwise. Continue turning the screws evenly one half turn counter clockwise until the pressure gauge on the double injector module is 35% less than the pressure gauge on the regulator module. Ensure that the tubing from one injector is placed into a graduated container containing 0.1 M HCl and the other into a graduated container containing 2% sodium thiosulfate. Loosen the hosecock clamps. Since there may be slight differences between the injectors and since the pressure reading after the injectors reflects an average pressure drop from both injectors, some addi-



**4.1.1** Attach sections of braided tubing (sterilized on inside and outside surfaces with chlorine and dechlorinated with thiosulfate as described in section 2.1.1a.10, 2.3.2) to the inlet and outlet ports of a cartridge housing module containing a 1MDS filter to be tested for viruses. If a prefilter was used, keep the prefilter and cartridge housing modules connected and attach the tubing to the inlet of the prefilter module and to the outlet of the cartridge housing module.

**4.1.2** Place the sterile end of the tubing attached to the outlet of the cartridge housing module into a sterile two liter glass or polypropylene beaker.

**4.1.3** Attach the free end of the tubing from the inlet port of the prefilter or cartridge housing modules to the outlet port of a sterile pressure vessel and attach the inlet port of the pressure vessel to a positive air pressure source. Add pressure to blow out any residual water from the cartridge housing(s). Open the vent/relief valve to release the pressure.

**4.1.4** Remove the top of the pressure vessel and pour 1000 mL of buffered 1.5% beef extract (pH 9.5, prewarmed to room temperature) into the vessel. Replace the top of the pressure vessel and close its vent/relief valve.

*Acceptable alternatives to the use of a pressure vessel include 1) the use of a peristaltic pump and sterile tubing to push the beef extract through the filter and 2) the addition of beef extract directly to the cartridge housing and the use of positive pressure to push the beef extract through the filter.*

**4.1.5** Open the vent/relief valve(s) on the cartridge housing(s) and slowly apply sufficient pressure to purge trapped air from them. Close the vent/relief valve(s) as soon as the buffered beef extract solution begins to flow from it. Turn off the pressure and allow the solution to contact the 1MDS filter for 1 min.

*Wipe up spilled liquid with disinfectant-soaked sponge. Carefully observe alternative housings without*

*vents to ensure that all trapped air has been purged.*

**4.1.6** Apply pressure to force the buffered beef extract solution through the filter(s) (see **Figure 14-8**).

*The solution should pass through the 1MDS filter slowly to maximize the elution contact period. When air enters the line from the pressure vessel, elevate and invert the filter housing to permit complete evacuation of the solution from the filters.*

**4.1.7** Turn off the pressure at the source and open the vent/relief valve on the pressure vessel. Place the buffered beef extract from the two liter beaker back into the pressure vessel. Replace the top of the pressure vessel and close its vent/relief valve. Repeat steps 4.1.5 - 4.1.6.



**Figure 14-8 Elution of 1MDS Filter**

(a) Turn off the pressure at the source and open the vent/relief valve on the pressure vessel. Thoroughly mix the eluate. Record the date and time of elution on a sample data sheet.

(b) Proceed to the Organic Flocculation Concentration Procedure (section 4.2) immediately. If the Organic Flocculation Concentration Procedure cannot be undertaken immediately, adjust the pH of the eluate to 7.0 to 7.5 with 1 M HCl and store the eluate at 4°C for up to 24 h or for longer periods at -70°C.

**4.2 ORGANIC FLOCCULATION CONCENTRATION PROCEDURE**

*Minimize foaming (which may inactivate viruses) throughout the procedure by not stirring or mixing faster than necessary to develop a vortex.*

**4.2.1** Place a sterile stir bar into the beaker containing the buffered beef extract eluate from the cartridge filter(s). Place the beaker onto a magnetic stirrer, and stir at a speed sufficient to develop a vortex.

**4.2.2** Insert a combination-type pH electrode into the beef extract eluate. Add 1 M HCl to the eluate slowly while moving the tip of the pipette in a circular motion away from the vortex to facilitate mixing. Continue adding 1 M HCl until the pH reaches  $3.5 \pm 0.1$  and then stir slowly for 30 min at room temperature (see **Figure 14-9**).

*The pH meter must be standardized at pH 4 and 7.*

*Sterilize electrodes before each use by immersing the tip of the electrode in 0.1% chlorine for at least 1 min.*

*Dechlorinate using a solution containing 2.5 mL of 2% sterile sodium thiosulfate per liter of sterile dH<sub>2</sub>O. Sterilize electrodes after each use by rinsing to remove particulates followed by immersion of the tip of the electrode in 0.1% chlorine again for at least 1 min.*

*Dechlorinate again using a solution containing 2.5 mL of 2% sterile sodium thiosulfate per liter of sterile dH<sub>2</sub>O.*

*A precipitate will form. If pH falls below 3.4, add 1 M NaOH to bring it back to  $3.5 \pm 0.1$ . Exposure to a pH below 3.4 may result in some virus inactivation.*



**Figure 14-9 Floc Formation**

**4.2.3** Remove the electrode from the beaker, and pour the contents of the beaker into a centrifuge bottle. Cap the bottle and centrifuge the precipitated beef extract suspension at  $2,500 \times g$  for 15 min at 4°C (see **Figure 14-10**). Remove and discard the supernatant.





